

Venturi Method Concept for Human Pulmonary Ventilation

Praneel John Titheradge^{1*} and Robert Robergs²

¹Charles Sturt University, Australia

²Queensland University of Technology, Australia

*Corresponding author: Praneel John Titheradge, Charles Sturt University, 8 Wellesley Court, Raglan, 2795, Bathurst NSW, Australia, Email: ptitheradge@csu.edu.au

Submission: 📅 November 14, 2017; Published: 📅 January 12, 2018

Introduction

No evidence exists for the application of a Venturi meter used as a pulmonary airflow sensor. This commentary article outlines the fluid dynamic principles behind the concept and rationale for the instrumentation processes involved for future validation of a Venturi air flow sensor, to be used for human pulmonary ventilation measurement.

The process of quantifying volumetric flow rate of the human breath is a common tool used within a subcategory of human physiology, called pulmonary ventilation. This method involves utilizing an airflow sensor, coupled with respiratory mouthpieces and tracheal tubing, to channel a given volume of breath through the sensor for measurement. There are many validated airflow devices, including the Pneu motachometer [1-9], Turbine flow meter [10], Hot-wire Anemometer [11-14], Pitot-static tube [15-17], as well

as the fixed or variable orifice tube [18,19]. Yet, no research has been conducted on the application, nor validation of the Venturi method to human pulmonary ventilation. Given its simple design, and ease of maintenance, the Venturi method provides a potentially inexpensive, reliable alternative to common methods that are prone to damage and relatively expensive to purchase and maintain. So how does it work?

The Venturi method operates by having a differential pressure transducer quantify the differential pressure (P_1-P_2) of air that occurs between two sections of a pipe of different diameter during fluid motion. This phenomenon is known as the Venturi effect and is described by the underlying fluid dynamics, known as the Bernoulli principle, which states that total pressure of a fluid remains a constant.

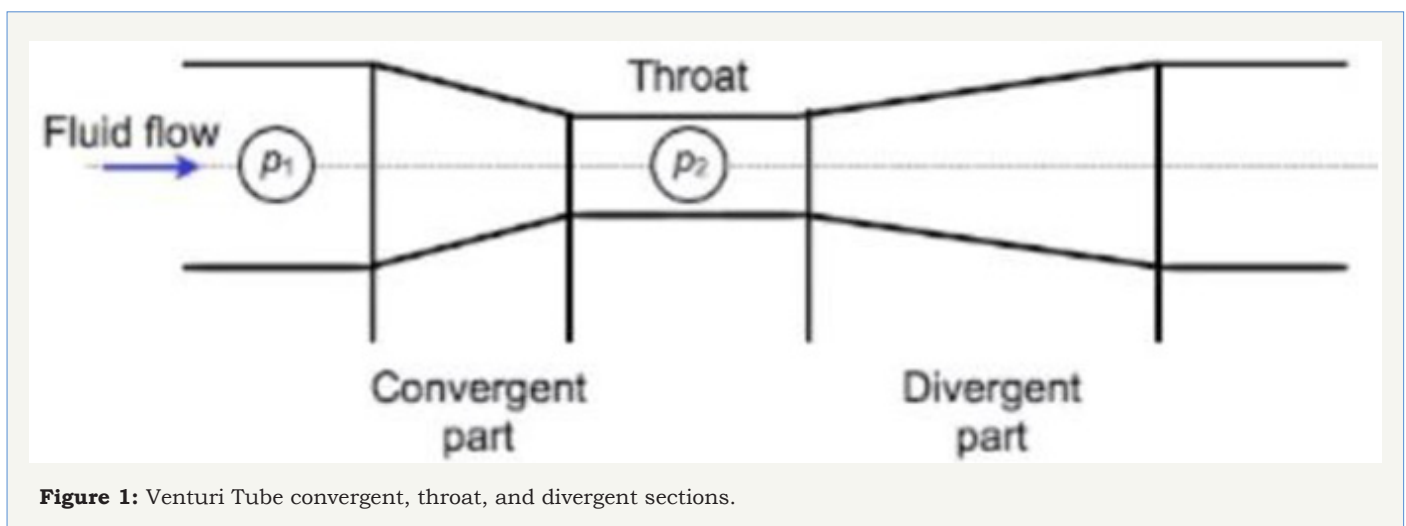


Figure 1: Venturi Tube convergent, throat, and divergent sections.

Bernoulli's theorem indicates that if a fluid flows horizontally so that gravitational potential energy remains negligible, then a change in the fluid's pressure is directly proportional to its velocity. Consider a small element of fluid of mass (m), which is acted on only by a pressure force (P) and not subject to the forces of gravity.

The fluid is regarded as isotropic and may differ from point to point in space, but does not differ with time. It is a well-known effect of Newton's laws of motion that when a particle of m moves under the influence of its weight (mg) (where g is the gravitational acceleration, $-9.8m/s^2$) and an additional force (F), from a point

(1) where its velocity is C_1 and its height is Z_1 , to another point (2) where its velocity is C_2 and its height is Z_2 , the work done by the additional force is equal to the change in kinetic and potential energy of the particle. In physics, kinetic energy is akin to the energy attributed to a fluid's velocity, whereas potential energy is akin to the hydrostatic pressure of a fluid. Static pressure however, refers to energy within a fluid that is measurable upon any point in a streamline, and is equal to total or atmospheric pressure when the fluid is stationary.

Venturi used Bernoulli's knowledge to demonstrate this relationship between a fluid's pressure and velocity by designing a pipe consisting of a convergent section, leading into a narrow throat section, followed by a divergent section where the pipe then returns into its original diameter (see Figure 1). The combination of these features is known as a Venturi Tube (fV), which can be used as a vacuum pump or a fluid measuring device (Figure 1).

As fluid flows through the fV, the transducer detects the pressure differential at p_1 and p_2 , a measurement of static pressure at each section of the pipe (see Figure 1). Because the fluid is flowing horizontally, hydrostatic pressure is negated. This means changes in fluid velocity can be detected by changes in static pressure. Given this relationship between fluid pressure and velocity can be measured, as well as the area of pipe at which the pressure was

taken, the volumetric flow rate can be quantified using equation 1.

$$V = A_1 \sqrt{\frac{2(P_1 - P_2)}{\rho[(A_1^2)^2 - 1]}} = \text{TheoreticalFlow Equation 1}$$

$V = \text{Volumetric Flow Rate}$

$A_2 = \text{Area of constricted pipe diameter (Throat section)}$

$P_1 - P_2 = \text{Differential pressure}$

$\rho = \text{fluid density}$

Establishing the configuration of a fV, that is, the area of the inlet, throat section, and outlet, can be conducted through computational methods to find the ideal setup for a particular application. For example, if a fV were to be used for paediatric pulmonary ventilation monitoring Vs. a fV used for adult high intensity exercise testing, such as during exercise testing with ventilation measurement and expired gas sampling, the configuration of the fV can be optimised for each condition initially through computational methods. This is demonstrated in Figure 2. which reveals $P_1 - P_2$ readings from two fV devices with 9.5mm and 12mm throat diameters matched to differential pressure transducers (Setra Systems, Inc. Boxborough, MA, USA, Model 267: 0-1KPa input & 0-7KPa input/ 10Volt output), during an airflow condition. The airflow rate was determined by a criterion device

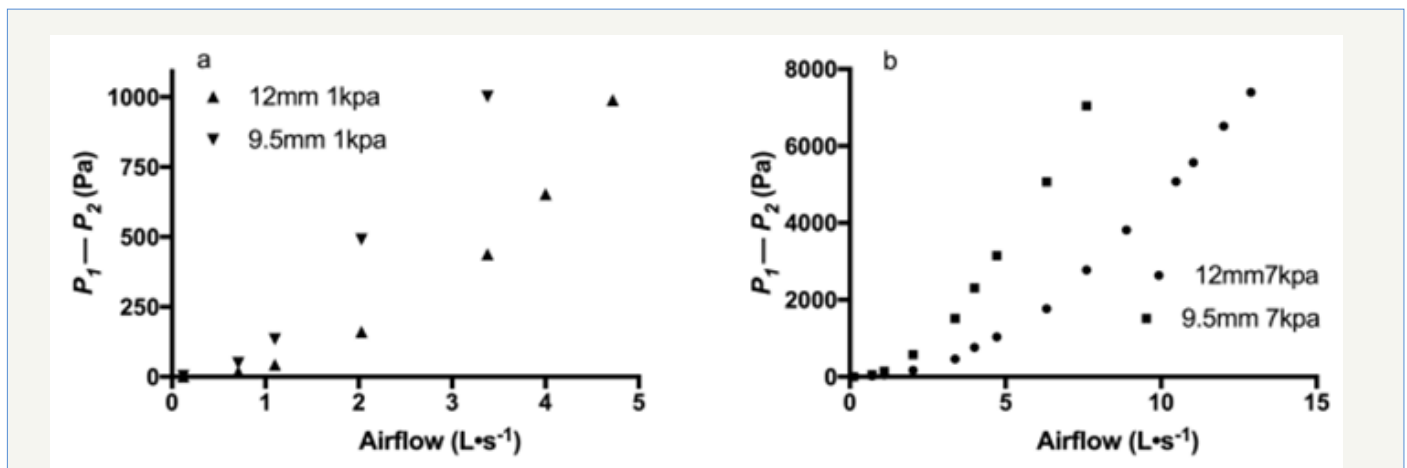


Figure 2: fV devices exposed to different airflow conditions. a) 12mm and 9.5mm throat fV specifications matched to 7kpa transducer. b) 12mm and 9.5mm throat fV specifications matched 1kpa transducer. Criterion airflow determined by Pneumotachometer.

(Pneumotachometer by Hans Rudolph, Inc. Shawnee, Kansas, USA). Based on the two fV instrumentation specifications, we can compare the measured $P_1 - P_2$ reading to a predicted $P_1 - P_2$ reading based on criterion airflow determination utilised in equation 1. In theory, a hypothetical value computed through equation 1 should be similar to actual measurements. Therefore, by performing algebraic substitution of equation 1, the effects from fV configuration and transducer specification can be revealed, which subsequently can be used for further instrumentation to optimise a fV device to meet application needs (Figure 2).

The Venturi equation utilises which takes into account the fluid density of air being measured. To compute fluid density, certain

environmental conditions must be known in order to improve the accuracy of volumetric airflow measurements. These include relative humidity, fluid temperature, and atmospheric pressure, which are used to compute equation 2, then subsequently used within equation 1.

$$\rho = \rho(1 + \chi) / (1 + 1.609\chi) \quad \text{Equation. 2}$$

$\rho = \text{density of moist air (kg/m}^3\text{)}$

$\rho da = \text{humidity ratio by mass (kg/m}^3\text{)}$

$\chi = \text{humidity ratio by mass (kg/kg)}$

1.609 = gas constant ratio between water vapour and air

All airflow sensor pulmonary ventilation measurements need to be converted to a standard measurement. For example, atmospheric, temperature, pressure, saturated conditions (L.min-1ATPS), converted to standard, temperature, pressure, dry conditions (L.min-1STPD), is carried out using equation 3. The standardisation of pulmonary ventilation measurements to constant conditions allows for comparison of tests with varying gas temperature, pressure and water vapour content between data collections.

$$VI_{STPD} = VI_{ATPS} \times (273 + 27T_{room}) \times (PB - 76P_{H2O}) \quad \text{Equation 3}$$

VI= Volume of Inspired Air (pulmonary ventilation)

273= Standard Temperature (0 °C = 273 °K)

T_{room} = Room Temperature

760= Standard Atmospheric Pressure (1 Atmosphere (Atm) = 760mmHg)

P_{H2O} = Water Vapour Pressure (mmHg)

BP= Barometric Pressure

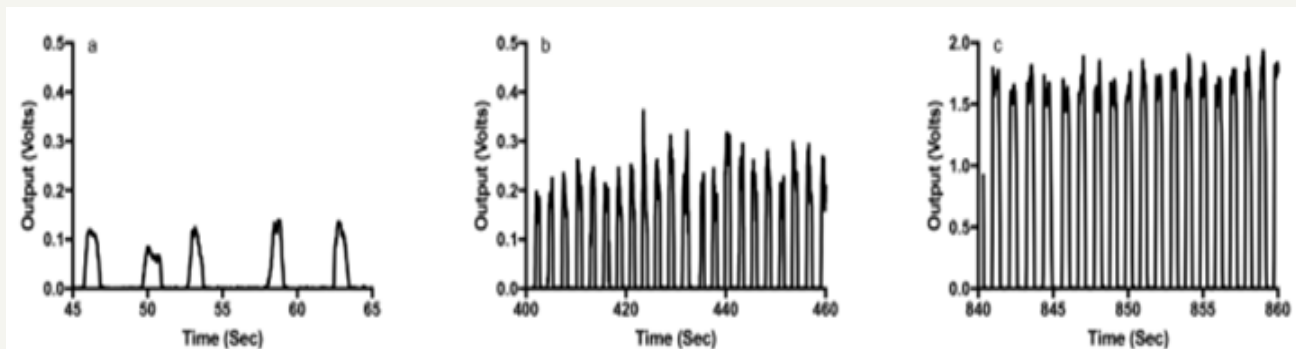


Figure 3: Continuous pulmonary ventilation monitoring during exercise to maximal exertion. A) resting ventilation b) Steady-state ventilation c) Pulmonary ventilation near maximal exertion.

The following subject data presented in Figure 3 is the continuous monitoring of pulmonary ventilation during an incremental physical exertion ramp test, conducted on a stationary cycle. The participant was setup with a pulmonary mouthpiece and one-way t-shaped valve (Hans Rudolph, Inc. Shawnee, Kansas, USA), with the fV device situated to measure inspired air. Independent

measurement of environmental conditions was carried out by a laboratory weather station device. Note the high frequency of breaths that can be observed during end of test (c). The fV signal reaches the baseline before each successive breath, indicating its dynamic performance is suitable for such applications (Figure 3).

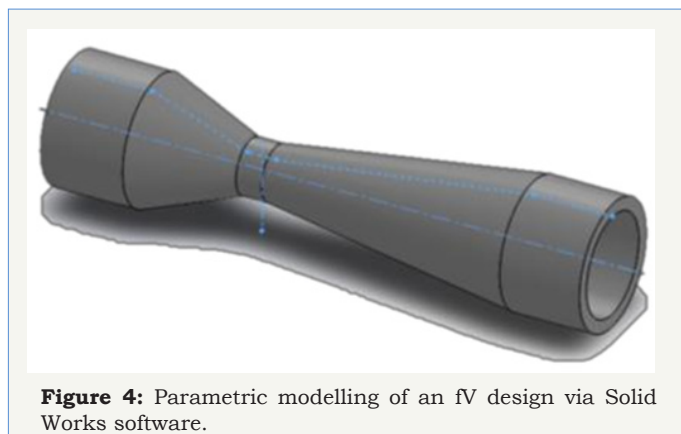


Figure 4: Parametric modelling of an fV design via Solid Works software.

Based on this rationale, we have continued research on developing the fV airflow sensor, through design and manufacturing via parametric modelling software and three-dimensional (3D) printing (See Figure 4).

We are working towards finalising results for computational design of an optimised fV for exercise testing, signal quality, dynamic performance, and clinical application. The fV device is simple and durable in design, readily accessible and easily cleaned and maintained, which can potentially reduce costs and minimise research and clinical disruptions due to damage.

Acknowledgements and Funding

This research endeavour has been funded by an Australian Government Ph.D. Research Training Program.

Conflict of Interest

This research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

References

1. Blumenfeld W, Turney S, Cowley R (1973) Mathematical model for flow in the heated fleisch pneumotachometer. Medical and Biological Engineering and Computing 11(5): 546-551.
2. Fincane KE, Egan BA, Dawson SV (1972) Linearity and frequency response of pneumotachographs. J Appl Physiol 32(1): 121-126.
3. Kreit JW, Sciruba FC (1996) The accuracy of pneumotachograph measurements during mechanical ventilation. Am J Respir Crit Care Med 154(4 pt 1): 913-917.
4. Ross SM, Kao FF (1961) Inexpensive pneumotachometer (PTM). J Appl Physiol 16(2): 380-381.
5. Strömberg N, Grönkvist MJ (1999) Improved accuracy and extended flow range for a Fleisch pneumotachograph. Med Biol Eng Comput 37(4): 456-460.
6. Turney S, Blumenfeld W (1973) Heated fleisch pneumotachometer: a

- calibration procedure. *J Appl Physiol* 34(1): 117-121.
7. Yeh MP, Adams TD, Gardner RM, Yanowitz FG (1987) Turbine flowmeter vs. Fleisch pneumotachometer: a comparative study for exercise testing. *J Appl Physiol* 63(3): 1289-1295.
 8. Yeh MP, Adams TD, Gardner RM, Yanowitz FG (1982) Computerized determination of pneumotachometer characteristics using a calibrated syringe. *J Appl Physiol Respir Environ Exerc Physiol* 53(1): 280-285.
 9. Zock JP (1981) Linearity and frequency response of Fleisch type pneumotachometers. *Pflügers Archiv* 391(4): p. 345-352.
 10. Frayne R, Holdsworth DW, Smith RF, Kasrai R, Larsen JP, et al.(1994) Turbine flow sensor for volume flow rate verification in MR. *Magn Reson Med* 32(3): 410-417.
 11. Bruner H (1947) The hot wire anemometer as a flowmeter. *Fed Proc* 6(1): 312.
 12. Caruso H (1973) The use of the hot-wire anemometer in respiratory processes. *Acta physiologica latino Americana* 24(1): 25-36.
 13. Lundsgaard J, Grønlund J, Einer-Jensen N (1979) Evaluation of a constant-temperature hot-wire anemometer for respiratory-gas-flow measurements. *Med Biol Eng Comput* 17(2): 211-215.
 14. Plakk P, Liik P, Kingisepp PH (1998) Hot-wire anemometer for spirometry. *Medical and Biological Engineering and Computing* 36(1): p. 17-21.
 15. Kirkness J, Verma M, McGinley BM, Erlacher M, Schwartz AR, et al.(2010) Pitot-tube flowmeter for quantification of airflow during sleep. *Physiol Meas* 32(2): 223-237.
 16. Porszasz J, Barstow TJ, Wasserman K (1994) Evaluation of a symmetrically disposed Pitot tube flowmeter for measuring gas flow during exercise. *J Appl Physiol* (1985) 77(6): 2659-2665.
 17. Wolf AR, Volgyesi GA (1987) A modified Pitot tube for the accurate measurement of tidal volume in children. *Anesthesiology* 67(5): 775-778.
 18. Fortuna ADO, Gurd JR (1999) Numerically based design of an orifice plate flowmetering system for human respiratory flow monitoring. *Ann Biomed Eng* 27(3): 356-365.
 19. Jitschin W (2004) Gas flow measurement by the thin orifice and the classical Venturi tube. *Vacuum* 76(1): 89-100.